



## **Abdominal CT Dose Examination for Adult Patient in Abuja and Keffi, Hospitals in Nigerian**

**U. Rilwan<sup>1\*</sup>, G. C. Onuchukwu<sup>2</sup>, L.K. Sabiu<sup>3</sup>, H. A. Abdullahi<sup>4</sup> and I. Umar<sup>5</sup>**

<sup>1</sup>Department of Physics, Nigerian Army University, P.M.B 1500, Biu, Borno State, Nigeria.

<sup>2</sup>Department of Mechanical Engineering, Nigerian Army University, P.M.B 1500, Biu, Borno State, Nigeria.

<sup>3</sup>Federal Medical Centre, Keffi P.M.B 004, Old Akwanga Road, Keffi, Nasarawa State, Nigeria.

<sup>4</sup>National Agency for Science and Engineering Infrastructure, Idu Industrial Area, P.M.B 391, Garki, Abuja-Nigeria.

<sup>5</sup>Department of Physics, Nasarawa State University, P.M.B 1022 Keffi, Nasarawa State, Nigeria.

### **Authors' contributions**

*This work was carried out in collaboration among all authors. Author UR designed the study, performed the statistical analysis, wrote the protocol and wrote the first draft of the manuscript. Authors UR, GCO and LKS managed the analyses of the study. Authors UR, HAA and IU managed the literature searches. All authors read and approved the final manuscript.*

### **Article Information**

DOI: 10.9734/AJARR/2020/v8i130191

#### Editor(s):

(1) Dr. Müge K. Davran, Associate Professor, Department of Agricultural Economics, Faculty of Agriculture, University of Çukurova, Adana, Turkey.

#### Reviewers:

(1) Punit Bansal, India.

(2) Mohammed Sidi, Bayero University Kano.

(3) Mohamed Abdelaziz El-Gamasy, Tanta University, Egypt.

Complete Peer review History: <http://www.sdiarticle4.com/review-history/53997>

**Original Research Article**

**Received 15 November 2019**

**Accepted 17 January 2020**

**Published 24 January 2020**

### **ABSTRACT**

This study has established local diagnostic reference levels (LDRLs). Dose report and scan parameters for abdomen was assessed during the period of seven months at the three study centres. Data on CT Dose index (CTDI<sub>w</sub>) and dose length product (DLP) available and achieved on CT scanner control console was recorded for a minimum of 10 average sized patients for each facility to established a local Diagnostic reference level (LDRLs) and radiation dose optimization Data was collected using a purposive sampling technique, from 131 adult patients weighing 70±3 kg) from Philip brilliance, Toshiba Alexion and General Electric (GE) CT scanners for this study. Third quartile values of the estimated LDRLs for CTDI<sub>w</sub> and DLP was determined as 12.7 mGy

\*Corresponding author: Email: rilwanusmanloko4@gmail.com;

and 560 mGy\*cm. The mean CTDIw obtained are lower to the reported data from the European Commission of 35 mGy. The mean DLP are comparably lower than all the reported value from the European commission of 780 mGy/cm. Therefore, there is no any clinical implication and hence CT dose optimization is recommended.

*Keywords: Radiation dose; MSCT; VGA; CTDIv; CTDIw; DLP; LDRL.*

## 1. INTRODUCTION

Computed tomography of the abdomen and pelvis is an application of computed tomography (CT) and is a sensitive method for diagnosis of abdominal diseases [1]. It is used frequently to determine stage of cancer and to follow progress [2]. It is also a useful test to investigate acute abdominal pain (especially of the lower quadrants, whereas ultrasound is the preferred first line investigation for right upper quadrant pain) [3]. Renal Stones, appendicitis, pancreatitis, diverticulitis, abdominal aortic aneurysm, and bowel obstruction are conditions that are readily diagnosed and assessed with CT [4]. CT is also the first line for detecting solid organ injury after trauma [5]. CT is an accurate technique for diagnosis of abdominal diseases [6]. Its uses include diagnosis and staging of cancer, as well as follow up after cancer treatment to assess response [7]. There are several advantages that CT has over traditional 2D medical radiography. First, CT completely eliminates the superimposition of images of structures outside the area of interest. Second, because of the inherent high-contrast resolution of CT, differences between tissues that differ in physical density by less than 1% can be distinguished. Finally, data from a single CT imaging procedure consisting of either multiple contiguous or one helical scan can be viewed as images in the axial, coronal, or sagittal planes, depending on the diagnostic task. This is referred to as multiplanar reformatted imaging [8]. CT is regarded as a moderate- to high-radiation diagnostic technique [9]. The improved resolution of CT has permitted the development of new investigations, which may have advantages; compared to conventional radiography, for example, CT angiography avoids the invasive insertion of a catheter [10]. CT colonography (also known as virtual colonoscopy or VC for short) is far more accurate than a barium enema for detection of tumors, and uses a lower radiation dose [11]. CT Virtual Colonoscopy is increasingly being used in the UK and US as a screening test for colon polyps and colon cancer and can negate the need for a colonoscopy in some cases. The radiation dose for a particular

study depends on multiple factors: volume scanned, patient build, number and type of scan sequences, and desired resolution and image quality [12]. In addition, two helical CT scanning parameters that can be adjusted easily and that have a profound effect on radiation dose are tube current and pitch. Computed tomography (CT) scan has been shown to be more accurate than radiographs in evaluating anterior interbody fusion but may still over-read the extent of fusion [13]. The radiation used in CT scans can damage body cells, including DNA molecules, which can lead to radiation-induced cancer [14]. The radiation doses received from CT scans is variable. Compared to the lowest dose x-ray techniques, CT scans can have 100 to 1,000 times higher dose than conventional X-rays [15]. However, a lumbar spine x-ray has a similar dose as a head CT [16]. Articles in the media often exaggerates the relative dose of CT by comparing the lowest-dose x-ray techniques (chest x-ray) with the highest-dose CT techniques. In general, the radiation dose associated with a routine abdominal CT has a radiation dose similar to three years average background radiation [17]. Some experts noted that CT scans are known to be "overused," and "there is distressingly little evidence of better health outcomes associated with the current high rate of scans" [18]. Early estimates of harm from CT are partly based on similar radiation exposures experienced by those present during the atomic bomb explosions in Japan after the Second World War and those of nuclear industry workers [19]. Some experts project that in the future, between three and five percent of all cancers would result from medical imaging [20]. An Australian study of 10.9 million people reported that the increased incidence of cancer after CT scan exposure in this cohort was mostly due to irradiation [21]. In this group, one in every 1,800 CT scans was followed by an excess cancer. If the lifetime risk of developing cancer is 40% then the absolute risk rises to 40.05% after a CT [22]. Some studies have shown that publications indicating an increased risk of cancer from typical doses of body CT scans are plagued with serious methodological limitations and several highly improbable results [23].

Concluding that no evidence indicates such low doses cause any long-term harm [24]. A person's age plays a significant role in the subsequent risk of cancer [25]. Estimated lifetime cancer mortality risks from an abdominal CT of a one-year-old are 0.1% or 1:1000 scans [26]. The risk for 40 years old patient is half that of 20 years old patient with substantially less risk in future [27,28].

The International Commission on Radiological Protection estimates that the risk to a fetus being exposed to 10 mGy (a unit of radiation exposure) increases the rate of cancer before 20 years of age from 0.03% to 0.04% (for reference a CT pulmonary angiogram exposes a fetus to 4 mGy)[27]. A 2012 review did not find an association between medical radiation and cancer risk in children noting however the existence of limitations in the evidences over which the review is based [29]. CT scans can be performed with different settings for lower exposure in children with most manufacturers of CT scans as of 2007 having this function built in [30]. Furthermore, certain conditions can require children to be exposed to multiple CT scans

[31,32]. This study assess Abdominal CT Dose Examination for Adult Patient in Abuja and Keffi, Hospitals in Nigerian.

## 2. MATERIALS AND METHODS

### 2.1 Materials

The materials requirements for the conduct of this research were included;

- i. Computer tomography scanner machines located at the study centers.
- ii. Data Collection Sheet
- iii. SPSS version (20) software for data analysis
- iv. Ethical clearance from the participated hospital that allowed this research to be conducted.

#### 2.1.1 Study Area

This section described exactly where the study centers were located, two of the study centers were located in Abuja and the remaining one located in Keffi as shown in Fig. 1 & 2.



Fig. 1. Map of Federal Capital Territory (FCT) Abuja, Showing the Study Area

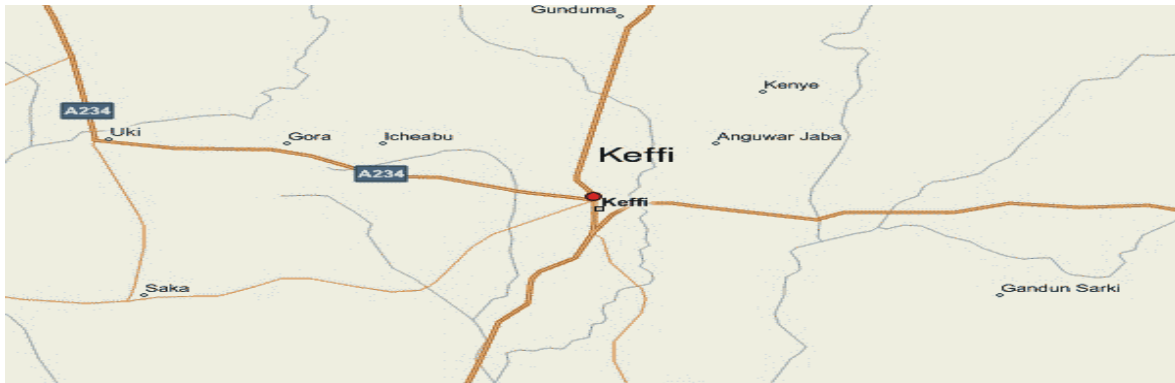


Fig. 2. Map of Keffi Showing the Study Area

**2.2 Methods**

The study adopted a retrospective and quantitative design to determine the absorbed radiation dose to patient undergoing CT scan of the abdomen. A quantitative design was appropriated because the study involved the uses of numerical data.

**2.2.1 Study population**

The study consisted of all adult patients that attended for CT scans examinations of abdomen. A simple size (45) participant patient was recruited for abdominal CT in the study. This was obtained through selection of 15 participants from centre A, 20 participants from centre B and 10 participants from centre C that come for CT examination on abdomen in center A, B and C respectively.

**2.2.2 Data collection**

The data was collected with the assistant of the CT radiographers who are well trained on how to collect the data. It was collected by the use data sheet which was used to record the data and Video Graphic Array which was use to display the result.

**2.2.3 Inclusion criteria**

- i. Only adult patients weighing in the range of 67 to 73 kg were included in the study [33].
- ii. Only adult patients that attended for routine CT scans of abdominal CT scan examination was considered.

Data was acquired on a CT scanner that was calibrated by the Nigeria Nuclear Regulatory Authority (NNRA) 2009, 2015 and 2014 for centre A, B and C respectively.

**2.2.4 Exclusion criteria**

- i. Patient that attended for non-routine CT procedure such as CT angiography, CT colonography.
- ii. Patients with weight above or below the specified limit [34].
- iii. CT scanner that was not calibrated by the Nigeria Nuclear Regulatory Authority (NNRA) 2009, 2015 and 2014 for centre A, B and C respectively.

**2.3 Data Analysis**

According to Karthikeyan and Chegu [35], the MSAD for non-spiral scans can be estimated from the CTDI by the equation:

$$MSAD = \frac{NXT}{I} (CTDI) \tag{1}$$

Where N is the number of scans, T is the nominal scan with (mm), and I is the distance between scans (mm). For MSCT system, N X T is the total nominal scan width, and I correspond to the patient table movement during 1 gantry rotation. According to the work of Seeram [36], the MSAD for spiral scans can be expressed as:

$$MSAD = \frac{I}{Pitch} (CTDI) \tag{2}$$

CTDI<sub>vol</sub>

According to Ling [37], CTDI<sub>vol</sub> for single-Slice scanners is defined as:

$$CTDI_{vol} = \frac{NXT}{I} (CTDIw) \tag{3}$$

When N is the number of scans, T is the nominal scan width (mm) and I is the distance between scans (AAPS). Also, CTDI<sub>vol</sub> for MSCT is defined as:

$$CTDI_{vol} = \frac{I}{Pitch} (CTDIw) \tag{4}$$

**3. RESULTS AND DISCUSSION**

**3.1 Result**

This section presents the data collected from the respective study centers as well as further evaluations for effective interpretations.


**3.2 Result Analysis**

In order to analyze the results obtained and presented in Table 1, charts were plotted and comparison was made with European Commission for all the CT Dose Measurement Parameters.


**3.3 Discussion**

This study determined the CTDIw and DLP for adult pertinent undergoing routine AbdominalCT scan in three Nigerian hospitals one located in Keffi, Nasarawa State while the other two are located in Abuja Federal Capital territory (FCT). Potential Local diagnostic reference levels were established.


From the result obtained above, Abdominal CT at centre (A& B) has the higherCTDIwabd DLP value followed by centre (C) then centre (B) respectively.

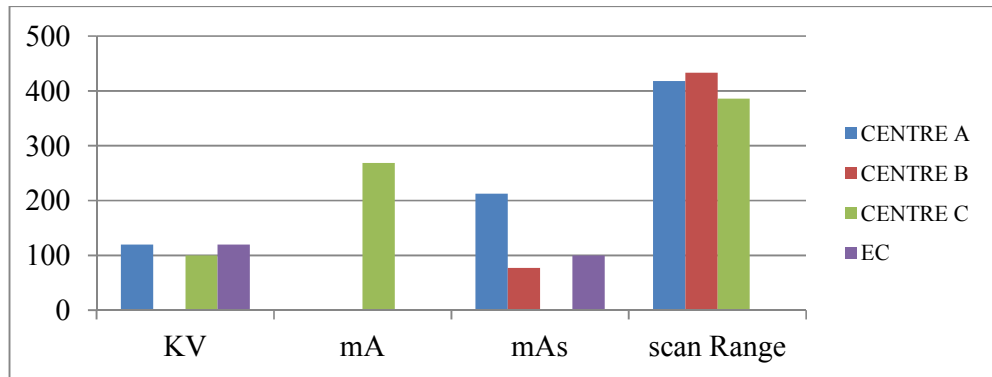


**Fig. 3. Comparison of Abdominal CT Scans Parameters between the Study Centres**

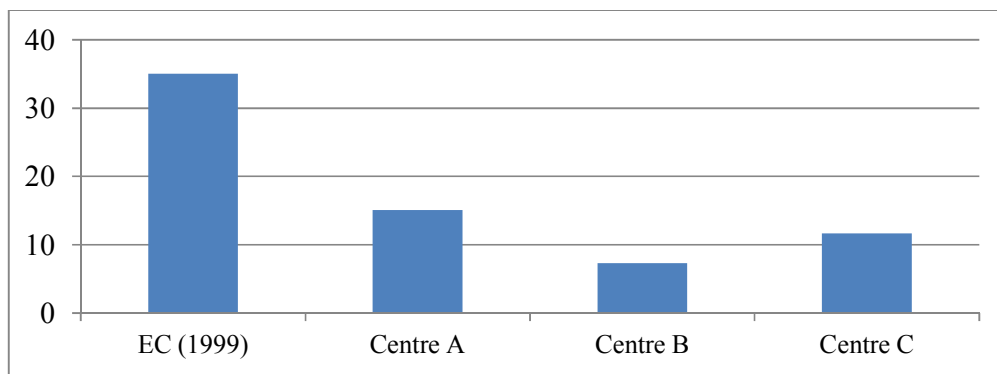

**Fig. 4. Comparison of Abdominal CTDIw (mGy) with European Commission for the study centres**

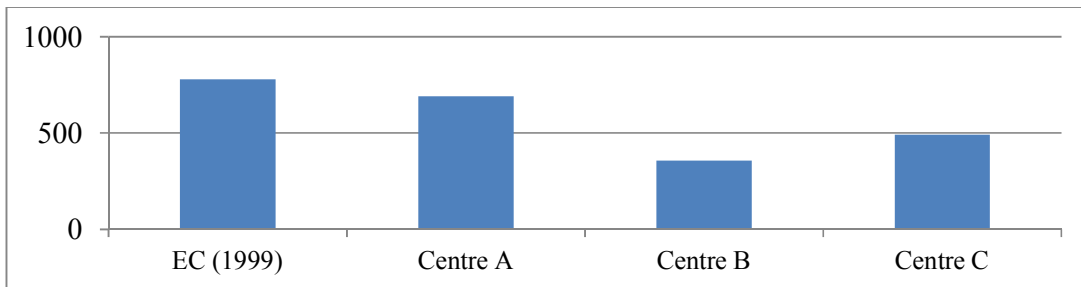

**Fig. 5. Comparison of Abdominal IDLP (mGy\*cm) with European Commission for the study centres**

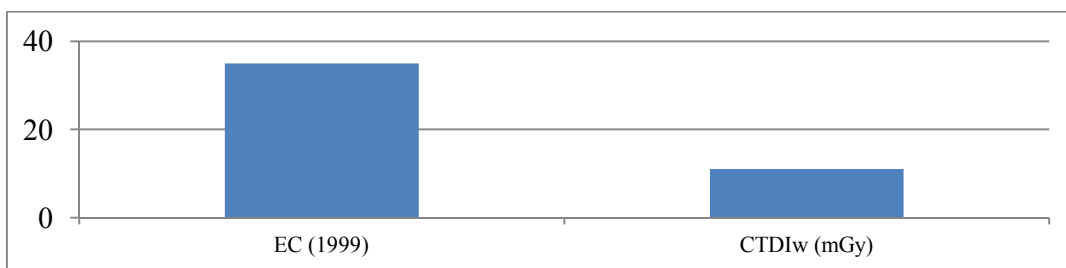

**Fig. 6. Comparison of mean Abdominal CTDIw (mGy) with European Commission**

**Table 1. Description of the Scanners for all Centres**


Centres	Scanner	Model	Number of Slides	Manufactured Year	Installed Year
A	Phillip	Brilliance	16	2008	2009
B	Simen	Alexion	32	2015	2015
C	General Electric	Bright Speed	16	2008	2014

**Table 2. Patients Description**

Centres	Av. Age (years)	Av. Weight (Kg)	No. of Male	No. of Female	Total No. of Patients
A	49.3±12.7	71.6±20.9	6	10	16
B	50.3±11.3	81.7±27.6	6	14	20
C	50.3±9.6	52.6±11.6	6	9	15

**Table 3. Scan parameters for all centres**

Scan parameters Centres	kV	mA	mAs	Scan Range	CTDIw (mGy)	DLP (mGy*cm)
A	120	NA	212.5±9.7	418.3±18.8	15.1±0.60	689.6±43.98
B	100	NA	76.9±43.0	433.0±63.0	7.3±4.67	356.7±248.15
C	120	268.9±113.5	NA	385.9±35.5	11.7±3.95	491.7±134.77
Mean					11.0±3.6	500.9±173.5

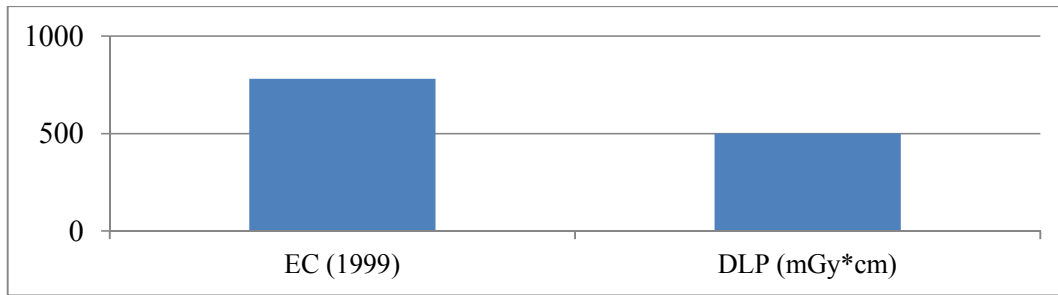

**Fig. 7. Comparison of mean Abdominal DLP (mGy\*cm) with European Commission**

In comparison with the European Commission values, it can be seen clearly from Figs. 4 and 5 that all the CTDI and DLP values are lower than the EC (European Commission) values.

Since the mean in Figs. 6 and 7 shows that the values for both CTDI and DLP are lower than the European Commission values.

#### **4. CONCLUSION AND RECOMMENDATION**

##### **4.1 Conclusion**

From this study, it can be concluded that the CTDI and the DLP in most of the study centres are within or below the values in the European Commission Report. Therefore, there may not be serious clinical implication on the participants in the study centres.

##### **4.2 Recommendation**

CT dose optimization and further researches is recommended.

#### **DISCLAIMER**

The products used for this research are commonly and predominantly use products in our area of research and country. There is absolutely no conflict of interest between the authors and producers of the products because we do not intend to use these products as an avenue for any litigation but for the advancement of knowledge. Also, the research was not funded by the producing company rather it was funded by personal efforts of the authors.

#### **CONSENT**

As per international standard or university standard written patient consent has been collected and preserved by the author(s).

#### **ETHICAL APPROVAL**

Ethical clearance from the participated hospital that allowed this research to be conducted.

#### **COMPETING INTERESTS**

Authors have declared that no competing interests exist.

#### **REFERENCES**

1. Lee HK, Park SJ, Yi BH, Multidetector CT reveals diverse variety of abdominal hernias. *Diagnostic Imaging*. 2010;27-31.
2. Brenner DJ, Hall EJ. Computed tomography – an increasing source of radiation exposure. *Engl. J. Med.* 2016; 2277–84.
3. Zabic S, Wang Q, Morton T, Brown KMA low dose simulation tool for CT systems with energy integrating detectors. *Medical Physics*. 2013;31-102.
4. Brian R, Subach MD, F.A.C.S. reliability and accuracy of fine-cut computed tomography scans to determine the status of anterior interbody fusions with metallic cages. 2012;12-18.
5. Redberg Rita F, Smith-B, Rebecca A. We are giving ourselves cancer. 2014;23-24.
6. Health, center for devices and radiological. Medical X-ray imaging - What are the radiation risks from CT. Available:www.fda.gov Archived from the original on 5 November 2013. Retrieved 1 May 2018
7. (ACR). Radiological Society of North America (RSNA) and American College of Radiology. Patient Safety - Radiation Dose in X-Ray and CT Exams. Available:radiologyinfo.org. Archived from the original on 14 March 2018. Retrieved 1 May 2018

8. Mathews JD, Forsythe AV, Brady Z, Butler MW, Goergen SK, Byrnes GB, Giles GG, Wallace AB, Anderson PR, Guiver TA, McGale P, Cain TM, Dowty JG, Bickerstaffe AC, Darby SC. Cancer risk in 680 000 people exposed to computed tomography scans in childhood or adolescence: Data linkage study of 11 million Australians. *BMJ*. 2013;23-60.
9. Sasieni PD, Shelton J, Ormiston-Smith N, Thomson CS, Silcocks PB. What is the lifetime risk of developing cancer? the effect of adjusting for multiple primaries. *British Journal of Cancer*. 2011;460-465.
10. Eckel LJ, Fletcher JG, Bushberg JT, McCollough CH. Answers to common questions about the use and safety of CT Scans. *Mayo Clinic Proceedings*. 2015; 1380-1392.
11. Expert opinion: Are CT scans safe. *Science Daily*; 2018. Retrieved 2019-03-14.
12. No evidence that CT scans, X-rays cause cancer. *Medical News Today*; 2016. Retrieved 2019-03-14
13. Furlow B. Radiation dose in computed tomography. *Radiologic Technology*. 2010; 437-50.
14. Davies HE, Wathen CG, Gleeson FV. The risks of radiation exposure related to diagnostic imaging and how to minimise them. *BMJ*. 2011,9-47.
15. Baysson H, Etard C, Brisse HJ, Bernier MO. Diagnostic radiation exposure in children and cancer risk: Current knowledge and perspectives. *Archives de Pédiatrie*. 2012;64-73.
16. Semelka RC, Armao DM, Elias J, Huda W. Imaging strategies to reduce the risk of radiation in CT studies, including selective substitution with MRI. *Journal of Magnetic Resonance Imaging*. 2007;900-9.
17. Larson DB, Rader SB, Forman HP, Fenton LZ. Informing parents about CT radiation exposure in children. *Am J Roentgenol*. 2007;271-5.
18. Smith-Bindman R, Lipson J, Marcus R, Kim KP, Mahesh M, Gould R, Berrington de González A, Miglioretti DL. Radiation dose associated with common computed tomography examinations and the associated lifetime attributable risk of cancer. *Arch. Intern. Med*. 2009;2078-86.
19. Berrington de González A, Mahesh M, Kim KP, Bhargavan M, Lewis R, Mettler F, Land C. Projected cancer risks from computed tomographic scans performed in the United States in 2007. *Arch. Intern. Med*. 2009;2071-7.
20. Hasebroock KM., Serkova NJ. Toxicity of MRI and CT contrast agents. *Expert Opinion on Drug Metabolism & Toxicology*. 2009;403-16.
21. CT Screening (PDF). *hps.org*. Archived from the original(PDF); 2016. Retrieved 1 May 2018.
22. Polo SE, Jackson SP. Dynamics of DNA damage response proteins at DNA breaks: A focus on protein modifications. *Genes Dev*. 2011;409-33.
23. The measurement, reporting, And management Of radiation dose In Ct archived 2017-06-23 at the wayback machine It is a single dose parameter that reflects the risk of a nonuniform exposure in terms of an equivalent whole-body exposure; 2016.
24. Hill B, Venning AJ, Baldock C. A preliminary study of the novel application of normoxic polymer gel dosimeters for the measurement of CTDI on diagnostic X-ray CT scanners. *Medical Physics*. 2005; 1589-1597.
25. Galloway RL Jr. Introduction and historical perspectives on image-guided surgery. In Golby, AJ (ed.). *Image-Guided Neurosurgery*. Amsterdam: Elsevier. 2015; 3-4.
26. Tse VCK, Kalani MYS, Adler JR. Techniques of stereotactic localization. In chin, LS; Regine, WF (eds.). *Principles and practice of stereotactic radiosurgery*. New York: Springer. 2015;28-29.
27. Saleh H, Kassas B. Developing stereotactic frames for cranial treatment. In benedict, SH; schlesinger, DJ; Goetsch, SJ; Kavanagh, BD (eds.). *Stereotactic Radiosurgery and Stereotactic Body Radiation Therapy*. Boca Raton: CRC Press. 2015;156-159.
28. Khan FR, Henderson JM. Deep brain stimulation surgical techniques. In Lozano, AM; Hallet, M (eds.). *Brain Stimulation: Handbook of Clinical Neurology*. 116. Amsterdam: Elsevier. 2013;28-30.
29. Arle J. Development of a classic. The toddwells apparatus, the BRW and the CRW Stereotactic Frames. In Lozano, AM; Gildenberg, PL; Tasker, RR (eds.). *Textbook of stereotactic and functional neurosurgery*. Berlin: Springer-Verlag. 2009;456-461.
30. Brown RA, Nelson JA. Invention of the N-localizer for stereotactic neurosurgery and



- its use in the Brown-Roberts-Wells stereotactic frame. *Neurosurgery*. 70 (2 supplement operative): 2012;173–176.
31. Furlow B. Radiation dose in computed tomography. *Radiologic Technology*.2010; 437–50.
32. EC. Guidelines on quality criteria for diagnostic radiographic images. European Commission EUR 16261EN. Accessed 2009  
Available:<http://www.bookshop.europa.eu>
33. Shrimpton PC, Miller HC, Lewis MA, Dunn M. Doses from Computed Tomography (CT) examinations in the UK; 2003. Review Archived 2011-09-22 at the Wayback Machine.
34. Morin RL, Gerber TE, McCollough CH. Radiation dose in computed tomography of the heart. *Circulation*. 2003;917-922.
35. Karthikeyan D, Chegu D. Step by step CT scan (A practical guide for Residents and Technologist).New Delhi, India: Jaypee Brothers Medical Publisher. 2005; 32-33.
36. Seeram C. Physical principles, clinical applications and quality control. 3<sup>rd</sup> Ed. Westline Industrial Drive St. Louis, Missouri: Saunders Elsevier. 2009;5-6.
37. Ling P. Factors affecting image quality and radiation dose in MDCT; 2013. Accessed 2009  
Available: <http://www.gehealthcare.com>

---

© 2020 Rilwan et al.; This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

*Peer-review history:*  
*The peer review history for this paper can be accessed here:*  
<http://www.sdiarticle4.com/review-history/53997>